



Test Report: GSM160B20

160W AC-DC Reliable Green Medical Adaptor

■ DESIGN VERIFY TEST

Output Function Test

Input Function Test

Protection Function Test

Component Stress Test

■ SAFETY & E.M.C. TEST

Safety Test

E.M.C. Test

■ RELIABILITY TEST

ENVIRONMENT TEST

DESIGN VERIFY TEST

OUTPUT FUNCTION TEST

| NO | TEST ITEM | SPECIFICATION | TEST CONDITION | RESULT |
|--|-------------------------------|--------------------------------|--|------------------------------------|
| 1 | OUTPUT VOLTAGE(Max) TOLERANCE | V1: -4%~ 4% | I/P: 100VAC /264VAC O/P:FULL/ MIN. LOAD Ta:25°C | V1: -0.786%~ 0.944% |
| 2 | LINE REGULATION (Max) | V1: -1%~ 1% | I/P: 100VAC~ 264VAC O/P:FULL LOAD Ta:25°C | V1: -0.03%~ 0.03% |
| 3 | LOAD REGULATION(Max) | V1: -4%~ 4% | I/P: 230VAC O/P:FULL ~MIN LOAD Ta:25°C | V1: -0.786%~ 0.944% |
| 4 | OVER/UNDERSHOOT TEST | < ±5% | I/P: 230VAC O/P:FULL LOAD Ta:25°C | < ±5% |
| 5 | RIPPLE & NOISE(Max) | V1: 120mVp-p | I/P:230VAC O/P:FULL LOAD Ta:25°C | V1: 17.2mVp-p |
| <div style="display: flex; justify-content: space-around;"> <div style="width: 45%;"> <p>high frequency :</p> </div> <div style="width: 45%;"> <p>low frequency :</p> </div> </div> | | | | |
| 6 | SET UP TIME(Max) | 230VAC/2000ms 115VAC/2500ms | I/P : 230 VAC I/P : 115 VAC O/P : FULL LOAD Ta : 25°C | 230VAC/ 1660 ms 115VAC/ 1090ms |
| <div style="display: flex; justify-content: space-around;"> <div style="width: 45%;"> <p>INPUT=230VAC/50HZ @ FULL LOAD</p> <p>CH1 : Output Voltage CH2 : AC Input Voltage</p> </div> <div style="width: 45%;"> <p>INPUT=115VAC/60HZ @ FULL LOAD</p> <p>CH1 : Output Voltage CH2 : AC Input Voltage</p> </div> </div> | | | | |
| 7 | RISE TIME (Max) | 230VAC/50ms 115VAC/50ms | I/P : 230 VAC I/P : 115 VAC | 230VAC/ 17.2 ms 115VAC/ 19.0 ms |




| | | | |
|--|---------------------|--|---|
| | | O/P : FULL LOAD Ta : 25°C | |
| INPUT=230VAC/50HZ @ FULL LOAD | | INPUT=115VAC/60HZ @ FULL LOAD | |
| <p>CH1 : Output Voltage</p> | | <p>CH1 : Output Voltage</p> | |
| 8 | HOLD UP TIME (Typ.) | 230VAC/24ms 115VAC/24ms | I/P : 230 VAC I/P : 115 VAC O/P : FULL LOAD Ta : 25°C |
| | | 26.8ms 27.2ms | |
| INPUT=230VAC/50HZ @ FULL LOAD | | INPUT=115VAC/60HZ @ FULL LOAD | |
| <p>CH1 : Output Voltage CH2 : AC Input Voltage</p> | | <p>CH1 : Output Voltage CH2 : AC Input Voltage</p> | |
| 9 | DYNAMIC LOAD | V1: 2000mVp-p | I/P: 230VAC O/P: (1)FULL /50% LOAD 50%DUTY / 120HZ (2)FULL /50% LOAD 50%DUTY / 1KHZ Ta:25°C |
| | | 390mVp-p 390mVp-p | |
| FULL /50% LOAD 50%DUTY / 120HZ | | FULL /50% LOAD 50%DUTY / 1KHZ | |
| | | | |

INPUT FUNCTION TEST


| NO | TEST ITEM | SPECIFICATION | TEST CONDITION | RESULT |
|----|-----------------------|-----------------------------|---|--|
| 1 | INPUT VOLTAGE RANGE | 80VAC~264VAC | I/P:TESTING O/P:FULL LOAD Ta:25°C | 66.650V~264V |
| | | | I/P: LOW-LINE-3V=97 V HIGH-LINE+15%=300 V O/P:FULL/MIN LOAD (PLEASE CHECK DERATING CURVE) ON: 30 Sec OFF: 30 Sec 10MIN (POWER ON/OFF NO DAMAGE) | TEST:OK |
| 2 | INPUT FREQUENCY RANGE | 47HZ ~63 HZ NO DAMAGE | I/P:100 VAC ~264 VAC O/P:FULL~MIN LOAD Ta:25°C | TEST: OK |
| 3 | INPUT CURRENT (Typ.) | 230V/ 1A 115V/ 1.85A | I/P : 230 VAC I/P : 115 VAC O/P : FULL LOAD Ta : 25°C | I =0.771A/ 230VAC I =1.508A/ 115VAC |
| 4 | LEAKAGE CURRENT | <0.1 mA / 264 VAC | I/P : 264 VAC O/P : Min LOAD Ta : 25°C | L-FG : 0.073 mA N-FG : 0.073 mA |
| 5 | NO LOAD CONSUMPTION | < 0.15W | I/P : 115VAC I/P : 230VAC O/P : NO LOAD Ta : 25°C | < 0.0967 W < 0.1230 W |
| 6 | POWER FACTOR (Typ.) | 0.94/ 230VAC 0.98/115VAC | I/P : 230 VAC I/P : 115 VAC O/P : FULL LOAD Ta : 25°C | PF=0.95/230VAC PF=0.99/115VAC |

P.F vs LOAD

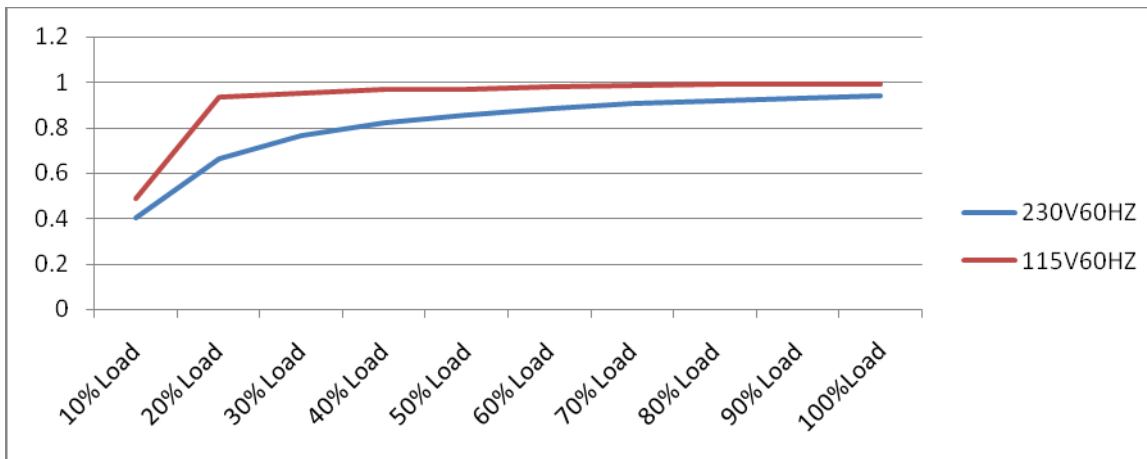

| | | | | |
|---|------------------|-------|---|--------|
| 7 | EFFICIENCY(Typ.) | 92.5% | I/P:230 VAC O/P:FULL LOAD Ta:25°C | 94.11% |
|---|------------------|-------|---|--------|

EFFICIENCY vs LOAD

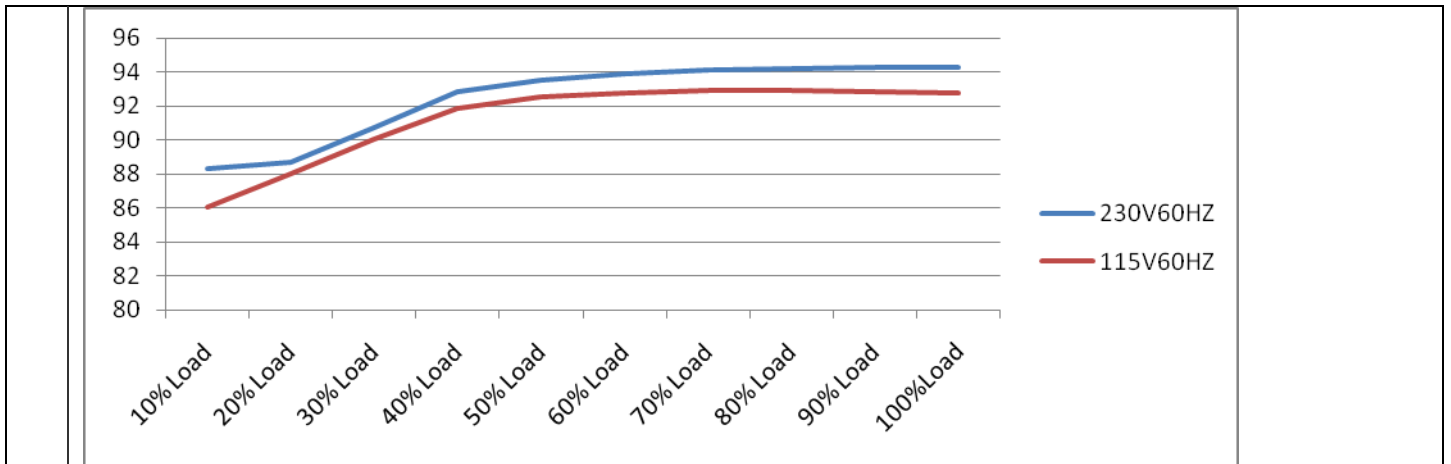

| | | | | |
|---|---|-------------------------------------|---|-------------------------------------|
| 8 | INRUSH CURRENT(Typ.) | 230V/110A 115V/90A COLD START | I/P : 230 VAC O/P : FULL LOAD Ta : 25°C | I =108A/ 230VAC I =49.2A/ 115VAC |
| | <p>INPUT=230VAC/50HZ @ FULL LOAD</p> <p>CH2 : AC Input Voltage CH4 : Input current (1V=1A)</p> <p>Ch4 Max 108 V</p> | | <p>INPUT=115VAC/ 60HZ @ FULL LOAD</p> <p>CH2 : AC Input Voltage CH4 : Input current (1V=1A)</p> <p>Ch4 Max 49.2 V</p> | |

PROTECTION FUNCTION TEST

| NO | TEST ITEM | SPECIFICATION | TEST CONDITION | RESULT |
|----|-----------------------------|---|--|--|
| 1 | OVER LOAD PROTECTION | 105%~ 150% | I/P: 264VAC I/P: 230VAC I/P: 100VAC O/P: TESTING Ta:25°C | 125.1%/ 264VAC 125.1%/ 230VAC 125.2%/100VAC PROTECTION TYPE : Hiccup mode,recovers automatically after fault condition is removed |
| 2 | OVER VOLTAGE PROTECTION | 21V~27V | I/P: 264VAC I/P: 230VAC I/P: 85VAC O/P: MIN LOAD Ta:25°C | 23.5V/ 264VAC 23.5V/ 230VAC 23.5V/ 90VAC PROTECTION TYPE : Shut down o/p voltage,re-power on to recover |
| 3 | OVER TEMPERATURE PROTECTION | Protection type : Protection type :Shut down o/p voltage,repower on to recover | I/P: 264VAC I/P: 90VAC O/P: FULL LOAD | O.T.P. Active Protection type :Shut down o/p voltage,repower on to recover |
| 4 | SHORT PROTECTION | SHORT EVERY OUTPUT 1 HOUR NO DAMAGE | I/P: 264VAC I/P: 90VAC O/P: FULL LOAD Ta:25°C | NO DAMAGE PROTECTION TYPE : Hiccup mode,recovers automatically after fault condition is removed |

COMPONENT STRESS TEST

| NO | TEST ITEM | SPECIFICATION | TEST CONDITION | RESULT |
|----|---|--|---|--|
| 1 | PWM Transistor (D to S) or (G to E) Peak Voltage | Q5 Rated : 12A/ 500V | I/P:High-Line +3V =267V AC ON/OFF VDS: O/P: (1)Full Load (2)Output Short (3) Full Load Continue Ta:25°C | VDS: (1) 452V (2) 456V (3) 446V |
| 2 | P.F.C Transistor (D to S) or (G to E) Peak Voltage | Q1 Rated : 16A/ 600V | I/P:High-Line +3V =267V AC ON/OFF VDS: O/P: (1)Full Load (2)Output Short (3) Full Load Continue Ta:25°C | VDS: (1) 520V (2) 522V (3) 512V |
| 3 | P.F.C DIODE | D1 Rated : 9 A/ 600V | I/P:High-Line +3V =267 V AC ON/OFF O/P: (1)Full Load (2)Output Short (3)Dynamic Load Full Load/ Min. Load 90%Duty/5KHz (4)Dynamic Load 100% Load/ Min. Load 50%Duty/120Hz Ta:25°C | (1) 422V (2) 424V (3) 428V (4) 430V |
| 4 | Diode Peak Voltage | Q101 Rated : 80A/ 75 V | I/P:High-Line +3V =267 V AC ON/OFF O/P: (1)Full Load (2)Output Short (3) Full Load Continue Ta:25°C | Q101: VDS: (1)45.6V (2)6.4V (3)45.8V |
| 5 | Input Capacitor Voltage | C5 Rated: : 150 μ / 420V 105°C | I/P:High-Line +3V =267 V O/P: (1)Full Load input on/off (2) Min load input on /Off (3)Full Load /Min load Change Ta:25°C | (1)416V (2)412V (3)402V |
| 6 | Control IC Voltage Test | IC U1 Rated : 38V -0.4V(MIN.) | I/P:High-Line +3V =267 V AC ON/OFF O/P(1)FULL LOAD (2) Output Short (3)O.L.P (4)O.V.P. Ta:25°C | (1) 28.6V (2) 20.0V (3) 20.0V (4) 29.5V |

SAFETY TEST

| NO | TEST ITEM | SPECIFICATION | TEST CONDITION | RESULT |
|----|----------------------|------------------------------|----------------------------------|--------------------------------------|
| 1 | WITHSTAND VOLTAGE | I/P-O/P: 4KVAC/min | I/P-O/P: 4.4 KVAC/min Ta:25°C | I/P-O/P:1.966mA NO DAMAGE |
| 2 | ISOLATION RESISTANCE | I/P-O/P:500VDC>100M Ω | I/P-O/P: 600 VDC Ta:25°C | I/P-O/P: 9999M Ω NO DAMAGE |

E.M.C TEST

| NO | TEST ITEM | SPECIFICATION | TEST CONDITION | RESULT |
|----|---|---|--|-------------------------------|
| 1 | HARMONIC | EN61000-3-2 CLASS A | I/P:230VAC/50HZ O/P:FULL LOAD Ta:25°C | PASS |
| 2 | CONDUCTION | EN55011 CLASS B | I/P : 230 VAC (50HZ) O/P : FULL/50% LOAD Ta : 25°C | PASS Test by certified Lab |
| 3 | RADIATION | EN55011 CLASS B | I/P : 230 VAC (50HZ) O/P : FULL LOAD Ta : 25°C | PASS Test by certified Lab |
| 4 | E.S.D | EN61000-4-2 AIR : 15KV / Contact : 8KV | I/P : 230 VAC/50HZ O/P : FULL LOAD Ta : 25°C | CRITERIA A |
| 5 | E.F.T | EN61000-4-4 INPUT : 2KV | I/P : 230 VAC/50HZ O/P : FULL LOAD Ta : 25°C | CRITERIA A |
| 6 | SURGE | EN61000-4-5 L-N : 1KV | I/P : 230 VAC/50HZ O/P : FULL LOAD Ta : 25°C | CRITERIA A |
| 7 | Test by certified Lab & Test Report Prepare | | | |

RELIABILITY TEST

ENVIRONMENT TEST

| NO | TEST ITEM | SPECIFICATION | TEST CONDITION | RESULT | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
|----|---|--|--|-------------------------|--------------------------|--------------------------|---|-----|--------|--------|---|-----|--------|--------|---|----|--------|--------|---|----|--------|--------|---|----|--------|--------|---|----|--------|--------|---|------|--------|--------|---|---------|--------|--------|---|------|--------|--------|----|------|--------|--------|----|-----|--------|--------|----|----|--------|--------|----|----|--------|--------|----|----|--------|--------|----|----|--------|--------|----|------|--------|--------|----|------|--------|--------|----|--------|--------|--------|----|-----|--------|--------|----|------|--------|--------|----|-----|--------|--------|----|----|--------|--------|----|-----|--------|--------|----|------|--------|--------|--|--|
| 1 | TEMPERATURE RISE TEST | MODEL : GSM160B15-R7B 1. ROOM AMBIENT BURN-IN : 1HRS I/P : 230VAC O/P : FULL LOAD Ta= 23.1 °C 2. HIGH AMBIENT BURN-IN : 1HRS I/P : 230VAC O/P : FULL LOAD Ta= 44.7 °C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | | <table border="1"> <thead> <tr> <th>NO</th> <th>Position</th> <th>ROOM AMBIENT Ta= 23.1 °C</th> <th>HIGH AMBIENT Ta= 44.7 °C</th> </tr> </thead> <tbody> <tr><td>1</td><td>LF1</td><td>45.8°C</td><td>66.6°C</td></tr> <tr><td>2</td><td>LF2</td><td>49.1°C</td><td>69.5°C</td></tr> <tr><td>3</td><td>L1</td><td>55.7°C</td><td>76.1°C</td></tr> <tr><td>4</td><td>L2</td><td>53.1°C</td><td>73.6°C</td></tr> <tr><td>5</td><td>D2</td><td>54.6°C</td><td>75.1°C</td></tr> <tr><td>6</td><td>C5</td><td>53.2°C</td><td>73.6°C</td></tr> <tr><td>7</td><td>RTH2</td><td>56.7°C</td><td>77.2°C</td></tr> <tr><td>8</td><td>T1 COIL</td><td>61.8°C</td><td>82.3°C</td></tr> <tr><td>9</td><td>C101</td><td>60.6°C</td><td>80.9°C</td></tr> <tr><td>10</td><td>C102</td><td>62.4°C</td><td>82.7°C</td></tr> <tr><td>11</td><td>BD1</td><td>55.6°C</td><td>75.7°C</td></tr> <tr><td>12</td><td>Q1</td><td>54.7°C</td><td>75.1°C</td></tr> <tr><td>13</td><td>D1</td><td>55.6°C</td><td>75.9°C</td></tr> <tr><td>14</td><td>Q6</td><td>55.7°C</td><td>76.2°C</td></tr> <tr><td>15</td><td>Q5</td><td>56.3°C</td><td>76.8°C</td></tr> <tr><td>16</td><td>Q101</td><td>60.5°C</td><td>81.4°C</td></tr> <tr><td>17</td><td>Q102</td><td>60.4°C</td><td>81.4°C</td></tr> <tr><td>18</td><td>T1Coil</td><td>57.3°C</td><td>77.3°C</td></tr> <tr><td>19</td><td>C13</td><td>61.6°C</td><td>81.4°C</td></tr> <tr><td>20</td><td>ZNR1</td><td>49.6°C</td><td>70.4°C</td></tr> <tr><td>21</td><td>C11</td><td>54.5°C</td><td>75.1°C</td></tr> <tr><td>22</td><td>R5</td><td>54.8°C</td><td>75.3°C</td></tr> <tr><td>23</td><td>C81</td><td>57.2°C</td><td>77.5°C</td></tr> <tr><td>24</td><td>U101</td><td>63.9°C</td><td>84.5°C</td></tr> </tbody> </table> | NO | Position | ROOM AMBIENT Ta= 23.1 °C | HIGH AMBIENT Ta= 44.7 °C | 1 | LF1 | 45.8°C | 66.6°C | 2 | LF2 | 49.1°C | 69.5°C | 3 | L1 | 55.7°C | 76.1°C | 4 | L2 | 53.1°C | 73.6°C | 5 | D2 | 54.6°C | 75.1°C | 6 | C5 | 53.2°C | 73.6°C | 7 | RTH2 | 56.7°C | 77.2°C | 8 | T1 COIL | 61.8°C | 82.3°C | 9 | C101 | 60.6°C | 80.9°C | 10 | C102 | 62.4°C | 82.7°C | 11 | BD1 | 55.6°C | 75.7°C | 12 | Q1 | 54.7°C | 75.1°C | 13 | D1 | 55.6°C | 75.9°C | 14 | Q6 | 55.7°C | 76.2°C | 15 | Q5 | 56.3°C | 76.8°C | 16 | Q101 | 60.5°C | 81.4°C | 17 | Q102 | 60.4°C | 81.4°C | 18 | T1Coil | 57.3°C | 77.3°C | 19 | C13 | 61.6°C | 81.4°C | 20 | ZNR1 | 49.6°C | 70.4°C | 21 | C11 | 54.5°C | 75.1°C | 22 | R5 | 54.8°C | 75.3°C | 23 | C81 | 57.2°C | 77.5°C | 24 | U101 | 63.9°C | 84.5°C | | |
| NO | Position | ROOM AMBIENT Ta= 23.1 °C | HIGH AMBIENT Ta= 44.7 °C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 1 | LF1 | 45.8°C | 66.6°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 2 | LF2 | 49.1°C | 69.5°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 3 | L1 | 55.7°C | 76.1°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 4 | L2 | 53.1°C | 73.6°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 5 | D2 | 54.6°C | 75.1°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 6 | C5 | 53.2°C | 73.6°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 7 | RTH2 | 56.7°C | 77.2°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 8 | T1 COIL | 61.8°C | 82.3°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 9 | C101 | 60.6°C | 80.9°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 10 | C102 | 62.4°C | 82.7°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 11 | BD1 | 55.6°C | 75.7°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 12 | Q1 | 54.7°C | 75.1°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 13 | D1 | 55.6°C | 75.9°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 14 | Q6 | 55.7°C | 76.2°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 15 | Q5 | 56.3°C | 76.8°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 16 | Q101 | 60.5°C | 81.4°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 17 | Q102 | 60.4°C | 81.4°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 18 | T1Coil | 57.3°C | 77.3°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 19 | C13 | 61.6°C | 81.4°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 20 | ZNR1 | 49.6°C | 70.4°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 21 | C11 | 54.5°C | 75.1°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 22 | R5 | 54.8°C | 75.3°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 23 | C81 | 57.2°C | 77.5°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 24 | U101 | 63.9°C | 84.5°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 2 | OVER LOAD BURN-IN TEST | NO DAMAGE 1 HOUR (MIN) | I/P : 230 VAC O/P : 130 % LOAD Ta : 25°C | TEST : OK | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 3 | LOW TEMPERATURE TURN ON TEST | TURN ON AFTER 2 HOUR | I/P : 264VAC/100VAC O/P : 100 % LOAD Ta= -35 °C | TEST : OK | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 4 | HIGH HUMIDITY HIGH TEMPERATURE HIGH VOLTAGE TURN ON TEST | AFTER 12 HOURS IN CHAMBER ON CONTROL 40 °C NO DAMAGE | I/P : 272 VAC O/P : FULL LOAD Ta= 40.1 °C HUMIDITY= 95 %R.H | TEST : OK | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 5 | TEMPERATURE COEFFICIENT | ± 0.03 %/°C (0-50°C) | I/P : 230 VAC O/P : FULL LOAD | ± 0.00367 %/°C (0-50°C) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |



| | | | |
|----|-----------------------------|---|---|
| 6 | STORAGE TEMPERATURE TEST | <ol style="list-style-type: none"> 1. Thermal shock Temperature : -40°C~ +85°C 2. Temperature change rate : 25°C / MIN 3. Dwell time low and high temperature : 30 MIN/EACH 4. Total test cycle : 5 CYCLE 5. Input/Output condition : STATIC | OK |
| 7 | THERMAL SHOCK TEST | <ol style="list-style-type: none"> 1. Thermal shock Temperature : -30°C~ +70°C 2. Temperature change rate : 25°C / MIN 3. Dwell time low and high temperature : 30 MIN/EACH 4. Total test cycle : 10 CYCLE 5. Input/Output condition : 230VAC/Full Load AC ON/OFF TEST turn on 58sec ; turn off 2sec | OK |
| 8 | VIBRATION TEST | <p>1 Carton & 1 Set</p> <ol style="list-style-type: none"> (1) Waveform : Sine Wave (2) Frequency : 10~500Hz (3) Sweep Time : 12min/sweep cycle (4) Acceleration : 2G (5) Test Time : 60min in each axis (X.Y.Z) (6) Ta : 25°C | TEST : OK |
| 9 | CAPACITOR LIFE CYCLE | <p>SUPPOSE C 102 IS THE MOST CRITICAL COMPONENT</p> <ol style="list-style-type: none"> (1) I/P : 230VAC O/P : FULL LOAD Ta= 25 °C LIFE TIME (2) I/P : 230VAC O/P : FULL LOAD Ta= 40 °C LIFE TIME (3) I/P : 230VAC O/P : 75% LOAD Ta= 40 °C LIFE TIME (4) I/P : 230VAC O/P : 50% LOAD Ta= 40 °C LIFE TIME | <ol style="list-style-type: none"> (1) 204288HRS (2) 79040HRS (3) 164768HRS (4) 258521HRS |
| 10 | MTBF | <p>MIL-HDBK-217F TOTAL FAILURE RATE : 239.1 KHRS</p> | |
| 11 | DMTBF/Accelerated Life Test | <p>Demonstration Mean Time Between Failure (Expected Life): Above 50,000 hours @ TA 50°C</p> | |

| TEST RESULT | TESTER | REVIEW | APPROVAL |
|-------------|--------|--------|----------|
| PASS | FRANK | GESG | WANGDZ |

2007/3/20 A50-S014